

1 SECTION 1.1

2 **INTRODUCTORY CHAPTERS**

3 CHAPTER 1.1.1.

4 **SAMPLING METHODS**

5 **INTRODUCTION**

6 *The starting point for the laboratory investigation of an animal disease is the taking of samples. This*
7 *first introductory chapter considers some of the general principles involved in sample collection,*
8 *submission and storage. Each of the disease chapters of this Terrestrial Manual provides specific*
9 *information on sample collection for that particular disease. Samples may be taken from animals or*
10 *the environment for a variety of purposes, such as disease diagnosis, disease surveillance, health*
11 *certification or monitoring the response to treatment or vaccination. The samples collected should*
12 *be appropriate for the intended purpose, and adequate in number and amount to provide*
13 *statistically valid results. Diagnostic laboratories require the submission of appropriate samples that*
14 *arrive at the laboratory in good condition. For disease diagnosis, the tissues sampled should be*
15 *representative of the condition being investigated and the lesions observed. Samples should be*
16 *taken with care, to avoid undue stress or injury to the animal or danger to the operator. Where*
17 *appropriate samples should be collected aseptically, and care should be taken to avoid cross-*
18 *contamination between samples.*

19 *The samples should be carefully packaged, labelled, and transmitted to the laboratory by the*
20 *fastest practicable method, with the appropriate temperature control. There are specific*
21 *requirements for the packaging and shipping of infectious substances, including diagnostic*
22 *specimens, which must be followed. If material is sent to a laboratory in another country, this*
23 *laboratory should be consulted in advance to ensure that it is willing to receive the material and to*
24 *obtain the appropriate import licence. All samples should be accompanied by a letter or submission*
25 *form, which includes the name and address of the submitter, the origin of the material, the relevant*
26 *history, animal identification and corresponding specimens, and the tests requested.*

27 **A. COLLECTION OF SAMPLES**

28 Before taking samples, careful consideration should be given to the purpose for which they are required. This will
29 determine the type and number of samples needed to provide valid results. When samples are taken from live
30 animals, care should be taken to avoid injury or distress to the animal or danger to the operator and attendants. It
31 may be necessary to use mechanical restraint, tranquillisation or anaesthesia. Whenever handling biological
32 material, from either live or dead animals, the risk of zoonotic disease should be kept in mind and precautions
33 taken to avoid human infection (see also Chapter 1.1.6. Human safety in the veterinary microbiology laboratory).
34 Post-mortem examinations should be carried out under as aseptic conditions as is practicable. Care should be
35 taken to avoid environmental contamination, or risk of spread of disease through insects or fomites.
36 Arrangements should be made for appropriate safe disposal of animals and tissues.

37 Considerable skill and care are required to decide on the correct samples to be sent to the laboratory. The
38 samples collected should be representative of the condition being investigated and the lesions observed.
39 Frequently, a combination of blood samples for serology and tissues from dead or culled animals for
40 microbiological culture will be required. Recommendations for transport are described later in this chapter.

41 The disease chapters in this *Terrestrial Manual* provide guidance on samples that should be collected so that
42 information will not be repeated here. In addition, procedures for sample collection and submission have been
43 prepared by National and International authorities (2, 4, 8, 11, 12). These publications provide detailed
44 recommendations of specific samples that should be collected from different species and for a wide variety of
45 suspected diseases. They also provide information on post-mortem procedures, lists of appropriate media, and
46 instructions on submission of samples. The laboratory that is going to perform the assay(s) should be contacted if
47 there are specific questions concerning the type of sample that should be collected.

48 1. Sample collection from live animals

49 a) Blood

50 Blood samples may be taken for haematology or for culture and/or direct examination for bacteria, viruses,
51 or protozoa, in which case it is usual to use anticoagulants, such as ethylene diamine tetra-acetic acid
52 (EDTA) or heparin. They may also be taken for serology, which requires a clotted sample. Blood plasma is
53 also used for some procedures. A blood sample is taken, as cleanly as possible, by venipuncture. In most
54 large mammals, the jugular vein or a caudal vein is selected, but brachial veins and mammary veins are also
55 used. In birds, a wing vein (brachial vein) is usually selected. In small laboratory animals, the vena
56 auricularis or vena retroorbitalis maybe useful to obtain blood samples or it maybe obtained by heart
57 puncture. Blood may be taken by syringe and needle or by needle and vacuum tube (not easy in delicate
58 veins but convenient in strong veins). Small quantities of blood are conveniently obtained by pricking with a
59 triangular, solid-pointed needle. Ideally the skin at the site of venipuncture should first be shaved (plucked)
60 and swabbed with 70% alcohol and allowed to dry.

61 For samples that are collected with anticoagulant, thorough mixing, using gentle agitation only, is necessary
62 as soon as the sample has been taken. It may also be necessary to make a smear of fresh blood on a
63 microscope slide; both thick and thin smears may be prepared. For serum samples, the blood should be left
64 to stand at ambient temperature (but protected from excessive heat or cold) for 1–2 hours until the clot
65 begins to contract. The clot can then be ringed round with a sterile rod and the bottles placed in a
66 refrigerator at 4°C. After several hours, or overnight, the sample can be centrifuged at about 1000 *g* for 10–
67 15 minutes and the serum can be decanted or removed with a pipette. In order to establish the significance
68 of antibody titres, paired serum samples will often need to be collected 14 days apart. An alternative method
69 for collecting and transporting blood that is to be used for serology is to place a drop of blood on to filter
70 paper, the blood is dried at room temperature and the sample can then be shipped unrefrigerated.

71 b) Faeces

72 At least 10 g of freshly voided faeces should be selected. Faeces for parasitology should fill the container
73 and be sent refrigerated to prevent hatching of parasite eggs and should arrive at the laboratory within
74 24 hours. Screw top containers or sterile plastic bags should be used for shipment; avoid tubes with rubber
75 stoppers as gas generated can result in blowing the stopper off the tube, ruining the integrity of the sample
76 and contaminating other samples in the package. An alternative and sometimes preferable method is to take
77 swabs from the rectum (or cloaca), taking care to swab the mucosal surface. The swabs should be visibly
78 coated with faecal material; however, samples collected with a swab are inadequate for parasitology. Care
79 should be taken when collecting swabs from small, delicate animals or birds to avoid injury to the animal;
80 small swabs are commercially available that should be used. Swabs should be transported in appropriate
81 transport medium. Faeces are best stored and transported at 4°C.

82 c) Skin

83 In diseases producing vesicular lesions, collect, if possible, 2 g of affected epithelial tissue as aseptically as
84 possible and place it in 5 ml phosphate buffered glycerine or Tris-buffered tryptose broth virus transport
85 medium at pH 7.6. Additionally, the vesicular fluid should be sampled where unruptured vesicles are
86 present; if possible, vesicular fluid should be aspirated with a syringe and placed in a separate sterile tube.
87 Plucked hair or wool samples are useful for surface feeding mites, lice and fungal infections. Deep skin
88 scrapings, using the edge of a scalpel blade, are useful for burrowing mites and, in birds, feather tips can be
89 taken for detection of viral antigen where Marek's disease is suspected.

90 d) Genital tract and semen

91 Samples may be taken by vaginal or preputial washing, or by the use of suitable swabs. The cervix or
92 urethra may be sampled by swabbing. Samples of semen are best obtained using an artificial vagina or by
93 extrusion of the penis and artificial stimulation. The sperm-rich fraction should be present in the sample and
94 contamination by antiseptic washing solutions should be avoided. Specific transport media and conditions
95 are often required.

96 e) Eye

97 A sample from the conjunctiva can be taken by holding the palpebra apart and gently swabbing the surface.
98 The swab is then put into transport medium. Scrapings may also be taken on to a microscope slide. The
99 handles of metal-handled swabs are useful for this, to ensure that sufficient cells are removed for
100 microscopic examination. Mucopurulent nasal and lacrimal discharges are rarely useful.

101 f) Nasal discharge (saliva, tears)

102 Samples may be taken with dacron, cotton or gauze swabs, preferably on wire handles as wood is inflexible
103 and may snap. It may be helpful if the swab is first moistened with transport medium. The swab should be
104 allowed to remain in contact with the secretions for up to 1 minute, then placed in transport medium and sent
105 to the laboratory without delay at 4°C. Long protected nasopharyngeal swabs should be used to collect
106 samples for some suspected viral infections.

107 g) Milk

108 Milk samples should be taken after cleansing and drying the tip of the teat, the use of antiseptics should be
109 avoided. The initial stream of milk should be discarded and a tube filled with the next stream(s), a sample of
110 bulk tank milk can be used for some tests. Milk for serological tests should not have been frozen, heated or
111 subjected to violent shaking. If there is going to be a delay in submitting them to the laboratory,
112 preservatives can be added to milk samples that are being collected for serological testing. If necessary,
113 milk for bacterial examination can be frozen.

114 2. Sample collection at post-mortem

115 Samples of tissue from a variety of organs can be taken at post-mortem. Detailed procedures for conducting a
116 post-mortem examination and collecting samples are described in most pathology text books; a guide to necropsy
117 procedures has been published (10). Post-mortem techniques are also included in some of the national guidelines
118 (2, 4, 8). A summary of these procedures will be provided here.

119 Animal health personnel should be trained in the correct procedures for post-mortem examination of the species
120 of animals with which they work. The equipment required will depend on the size and species of animal, but a
121 knife, saw and cleaver will be required, and also scalpel, forceps and scissors, including scissors with a rounded
122 tip on one blade, for opening intestines. A plentiful supply of containers appropriate to the nature of the sample
123 required should be available, along with labels and report forms. Containers should be fully labelled with the date,
124 tissue and animal identification. Special media may be required for transport of samples from the field. The
125 operator should wear protective clothing: overalls, washable apron, rubber gloves and rubber boots. Additionally,
126 if potential zoonotic diseases are being investigated, the post-mortem examination should be conducted in a
127 biological safety cabinet; if this is not possible, an efficient face mask and eye protection should be worn. If rabies
128 or transmissible spongiform encephalopathies (TSEs) are suspected, it is usual to detach the animal's head.

129 Tissues may be collected for microbiological culture, parasitology, biochemistry, histopathology and/or immuno-
130 histochemistry, and for detection of proteins or genome nucleic acids. The person conducting the post-mortem
131 examination should have sufficient knowledge of anatomy and pathology to select the most promising organs and
132 lesions for sampling. Each piece of tissue should be placed in a fully labelled separate plastic bag or sterile
133 screw-capped jar. Sterile instruments should be used for collecting specimens for microbiological culture and care
134 should be taken not to contaminate tissues with intestinal contents. Disinfectants should not be used on or near
135 tissues to be sampled for bacterial culture or virus isolation.

136 The tissues may be sent to the laboratory dry or in bacterial or virus transport medium, depending on the
137 examinations required. After collection, the samples for microbiological examination should be refrigerated until
138 shipped. If shipment cannot be made within 48 hours, the samples should be frozen; however, prolonged storage
139 at -20°C may be detrimental to virus isolation. For histopathology, blocks of tissue not more than 0.5 cm thick and
140 1–2 cm long are cut and placed in neutral buffered 4–10% formalin, which should be at least ten times the volume
141 of the tissue sample. For certain suspected diseases, larger portions of brain are required; the brain is sectioned
142 using a sagittal cut, half is submitted fresh, on ice, and the other half is submitted in 10% buffered formalin. For
143 scrapie, bovine spongiform encephalopathy and other TSEs, details of sample collection are provided in the
144 individual disease chapters in this *Terrestrial Manual*. Store and pack formalin-fixed tissues separately from fresh
145 tissues, blood and smears. Care should be taken to insure that formalin-fixed tissues are not frozen. Once fixed,
146 tissues can be removed from formalin and, as long as they are kept moist and protected (e.g. by wrapping in
147 formalin-soaked paper towels, then sealed in screw-capped jars), they can be forwarded to the laboratory without
148 formalin.

149 **3. Environmental and feed sampling**

150 Samples may be taken to monitor hygiene or as part of a disease enquiry. Environmental samples are commonly
 151 taken from litter or bedding and voided faeces or urine. Swabs may be taken from the surface of ventilation ducts,
 152 feed troughs and drains. This kind of sampling is particularly important in hatcheries, artificial insemination centres
 153 and slaughter houses in which specialised equipment is maintained. Samples may also be taken from animal
 154 feed, in troughs or bulk containers. Water may be sampled in troughs, drinkers, header tanks or from the natural
 155 or artificial supply.

156 **4. Honey bees**

157 Adult bees, either dead or moribund, may be collected in the vicinity of the colonies. Live bees should be killed by
 158 freezing. Brood samples are taken by removing a piece of brood comb that shows abnormalities. This should be
 159 wrapped in paper and placed in a box for transport to the laboratory.

160 **B. SAMPLE SIZE**

161 When investigating a case of clinical disease, the samples collected should be representative of the condition
 162 being investigated and the lesions observed. When developing a programme of surveillance and monitoring for
 163 animal health, some general statistical sampling methods should be used. These sampling methods are needed
 164 to perform the scientifically based surveys specified in the OIE *Terrestrial Animal Health Code* (9). It is possible to
 165 calculate how many animals should be sampled from a herd/flock of a certain size, to achieve a 95% probability of
 166 detecting infection assumed to be present in a certain percentage of the animals. The following formulae can give
 167 approximate numbers but a specific sampling program for the planned surveillance program should be based on
 168 complete formulas available in the references (1, 3, 11) or by the use of a program (FreeCalc) available off the
 169 internet: http://www.ausvet.com.au/content.php?page=res_software#freecalc.

170 The following formula could be used to calculate the sample size n to detect at least one infection with a test that
 171 has a 100% sensitivity and specificity; where α is the significance level and $1-\alpha$ is the level of confidence, p is the
 172 prevalence in the population. If disease were present in 5% of a herd of 500 animals, it would be necessary to
 173 sample 59 animals to be 95% confident of finding at least one positive, assuming that both the sensitivity and
 174 specificity of the test were 100%. As most diagnostic tests do not have specificity and sensitivity of 100%, the
 175 number of samples collected must be adjusted to the sensitivity and specificity of the test that will be used (see
 176 also Chapter I.1.3. Principles of validation of diagnostic assays for infectious diseases).

$$n = \frac{\ln(\alpha)}{\ln(1-p)}$$

177 In the above example $\alpha = 0.05$, $1-\alpha = 95\%$, $p = 0.05$ and $n = 59$

178 If the sensitivity (Se) is less than 100%, the above formula should be modified as follows:


$$n = \frac{\ln(\alpha)}{\ln(1-p \cdot Se)}$$

179 In the above example with $\alpha = 0.05$, $p = 0.05$, specificity (Sp) = 1 and $Se = 0.95$, a minimum of $n = 62$ animals
 180 instead of 59 would need to be sampled to have a probability of at least 0.95 of finding a positive animal. The
 181 increase in the sample size from 59 to 62 is due to the decrease in the sensitivity of the test from 1 to 0.95. The
 182 graph below gives the minimum sample size required for finding at least one positive for several sensitivity and
 183 prevalence combinations at $\alpha = 0.05$ and $Sp = 1$.

184 If the test is known to have a specificity of less than 1, the positive results should be confirmed by a test with a
 185 higher specificity. If the prevalence is very low and the test used has a specificity of less than 1, it is very possible
 186 that a positive test result is a false positive.

Sample Size Calculations

(Specificity= 1 Alpha=0.05)

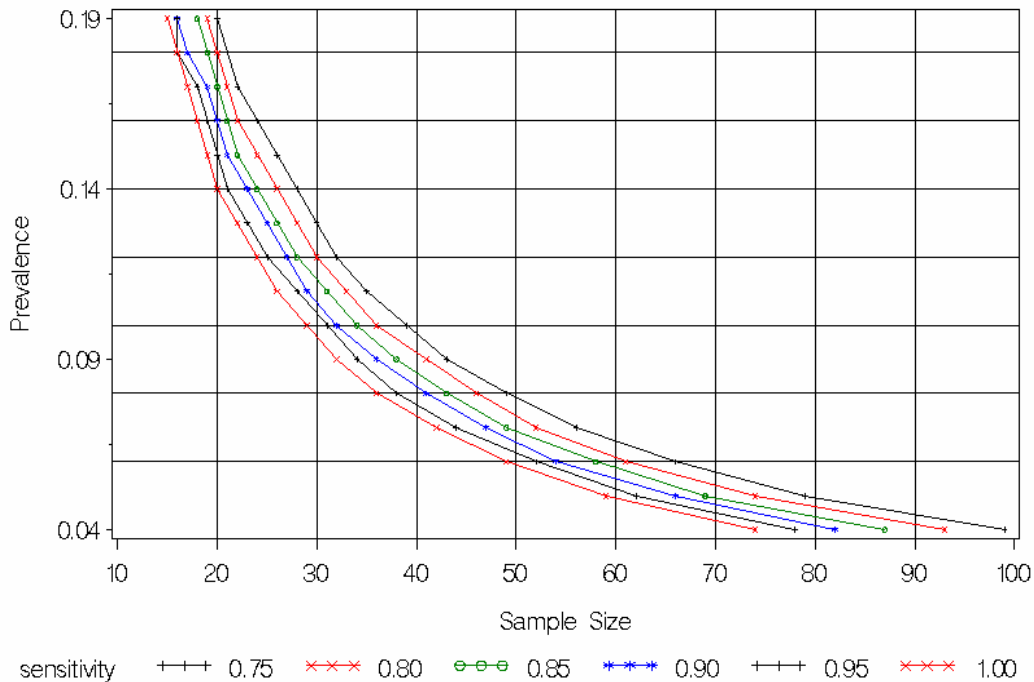

187

188

189

Fig. 1. Minimum sample size required to be 95% confident of finding infection at various sensitivity and prevalence combinations

190

C. INFORMATION TO BE SENT WITH SAMPLES

191

192

193

194

195

196

197

It is essential that individual samples be clearly identified using appropriate methods. Marking instruments should be able to withstand the condition of use, i.e. being wet or frozen. Pencil has a tendency to rub off containers and labels attached to plastic will fall off when stored at -70°C . Information and case history should always accompany the samples to the laboratory, and should be placed in a plastic envelope on the outside of the shipping container. The following are suggested items that should be addressed. It would be advisable to contact the receiving laboratory to determine if it has a submission form that it would like to have submitted with the samples or if it needs other information.

198

i) Name and address of owner/occupier where disease occurred, with telephone and fax numbers.

199

ii) Name, postal and e-mail address, telephone and fax numbers of the sender.

200

iii) Diseases suspected and tests requested.

201

iv) The species, breed, sex, age and identity of the animals sampled.

202

v) Date samples were collected and submitted.

203

vi) List of samples submitted with transport media used.

204

205

vii) A complete history would be beneficial for the laboratory and should be included if possible. Some of the components of the history are:

206

a) A list and description of the animals examined and the findings of the post-mortem examination.

207

208

b) The length of time sick animals have been on the farm; if they are recent arrivals, from where did they originate.

209

210

c) The date of the first cases and of subsequent cases or losses, with any appropriate previous submission reference numbers.

211

d) A description of the spread of infection in the herd or flock.

212

213

e) The number of animals on the farm, the number of animals dead, the number showing clinical signs, and their age, sex and breed.

- 214 f) The clinical signs and their duration including the condition of mouth, eyes and feet, and milk or egg
215 production data.
- 216 g) The type and standard of husbandry, including the type of feed available, possible contact with poison
217 or poisonous plants.
- 218 h) Any medication given to the animals, and when given.
- 219 i) Any vaccination given, and when given.
- 220 j) Other observations about the disease and husbandry

221 D. PACKAGING AND TRANSPORT OF SAMPLES

222 1. Approval to ship specimens

223 The laboratory that is going to receive the samples should be contacted to ensure that it has the capability to do
224 the testing requested and to see if there are any special packaging or shipping requirements. It is essential to
225 contact the receiving laboratory when material is sent to another country. A special import licence will usually be
226 required and must be obtained in advance for any biological material. This licence should be placed in an
227 envelope on the outside of the parcel.

228 2. Transportation of specimens

229 The specimens should be forwarded to the laboratory by the fastest method available. If they can reach the
230 laboratory within 48 hours, samples should be sent refrigerated. If dry ice is used, the additional packaging
231 requirements must be met. Infectious substances, which can include diagnostic specimens, are not permitted to
232 be shipped as checked luggage or as carry on luggage and must be shipped as cargo.

233 3. Packaging

234 The shipper should ensure that the specimens are packaged so they arrive at the laboratory in good condition
235 and there is no leakage during shipment. The International Air Transport Association (IATA), Dangerous Goods
236 Regulations (DGR) have explicit requirements for packaging and shipment of diagnostic specimens, by all
237 commercial means of air transport (5, 6). In many countries, similar requirements are applicable to ground
238 shipments and the postal service. These requirements for air transport are covered in detail in the IATA
239 publications, which are updated every year. The shipper is expected to know and follow the procedures outlined
240 in the current DGR. The following is a summary of the regulations at the time that this *Terrestrial Manual* went to
241 publication and it should only be used as a guide for shipping. It is anticipated that there will be major changes in
242 the DGR effective 1 January 2005. If there are significant changes in the DGR, a revised version of this chapter
243 will be posted on the OIE web site: www.oie.int. Shippers must also always check the latest version of the IATA
244 DGR prior to shipping diagnostic specimens. In addition, three of the National guidelines provide explicit
245 directions for packaging and shipping diagnostic specimens and are based on IATA requirements (2, 4, 8).

246 The DGR outline the procedures for the shipment of infectious substances, which can include diagnostic
247 specimens. Infectious substances are defined in the DGR as substances which are known or are reasonably
248 expected to contain pathogens. Pathogens are defined as micro-organisms (including bacteria, viruses,
249 rickettsiae, parasites, fungi) or recombinant micro-organisms (hybrid or mutant) that are known or reasonably
250 expected to cause disease in humans or animals.

251 The IATA (5, 6) lists the following exemption from the Dangerous Goods Regulations:

252 *Substances which do not contain infectious substances or substances which are unlikely to cause disease in*
253 *humans or animals are not subject to these regulations unless they meet the criteria for inclusion in another class.*

254 There are also exceptions for some Biological Products and the shipper of these products is referred to the IATA
255 Regulations for these requirements as some Biological Products are not exempted. The following is the DGR
256 definition of Biological Products (5, 6):

257 *Biological products are derived from living organisms. These are manufactured and distributed in accordance with*
258 *the requirements of appropriate national governmental authorities, which may have special licensing*
259 *requirements, and are used either for prevention, treatment, or diagnosis of disease in humans or animals, or for*
260 *development, experimental or investigational purposes related thereto. They include, but are not limited to,*
261 *finished or unfinished products such as vaccines and diagnostic products.*

262 The DGR state that infectious substances (including diagnostic specimens likely to contain animal or human
263 pathogens) are designated as UN 2814, UN 2900 or UN 3373.

264 Samples sent for diagnostic purposes should be designated as UN 2814 or UN 2900 if they include material
265 derived from humans or animals with a disease that can be readily transmitted and for which effective treatment
266 and preventative measures are not usually available¹. Infectious substances meeting this definition that affect
267 humans, including zoonotic agents, are designated UN 2814; those affecting animals only are designated
268 UN 2900.

269 Infectious substances shipped for diagnostic purposes that do not meet the criteria for assignment to UN 2814 or
270 UN 2900 are assigned to UN 3373 and designated as 'Diagnostic Specimens'.

271 The IATA DGR contain an indicative list of pathogens that must be assigned to UN 2814 or UN 2900 (Tables 1
272 and 2). The pathogens on these lists cannot be assigned to UN 3373 (5, 6).

273 **Table 1.** Infectious substances affecting humans that must be designated UN 2814

<i>Bacillus anthracis</i> (cultures only)	Japanese Encephalitis virus (cultures only)
<i>Brucella abortus</i> (cultures only)	Junin virus
<i>Brucella melitensis</i> (cultures only)	Kyasanur Forest disease virus
<i>Brucella suis</i> (cultures only)	Lassa virus
<i>Burkholderia mallei</i> – <i>Pseudomonas mallei</i> – Glanders (cultures only)	Machupo virus
<i>Burkholderia pseudomallei</i> – <i>Pseudomonas pseudomallei</i> (cultures only)	Marburg virus
<i>Chlamydia psittaci</i> – avian strains (cultures only)	<i>Mycobacterium tuberculosis</i> (cultures only)
<i>Clostridium botulinum</i> (cultures only)	Monkeypox virus
<i>Coccidioides immitis</i> (cultures only)	Nipah virus
<i>Coxiella burnetii</i> (cultures only)	Omsk hemorrhagic fever virus
Crimean-Congo hemorrhagic fever virus	Poliovirus (cultures only)
Dengue virus (cultures only)	Rabies virus
Eastern equine encephalitis virus (cultures only)	<i>Rickettsia prowazekii</i> (cultures only)
<i>Escherichia coli</i> , verotoxigenic (cultures only)	<i>Rickettsia rickettsii</i> (cultures only)
Ebola virus	Rift Valley fever virus
Flexal virus	Russian spring-summer encephalitis virus (cultures only)
<i>Francisella tularensis</i> (cultures only)	Sabia virus
Guanarito virus	Shigella dysenteriae type 1 (cultures only)
Hantaan virus	Tick-borne encephalitis virus (cultures only)
Hantaviruses causing hantavirus pulmonary syndrome	Variola virus
Hendra virus	Venezuelan equine encephalitis virus
Hepatitis B virus (cultures only)	West Nile virus (cultures only)
Herpes B virus (cultures only)	Yellow fever virus (cultures only)
Human immunodeficiency virus (cultures only)	<i>Yersinia pestis</i> (cultures only)
Highly pathogenic avian influenza virus (cultures only)	

1 The definition that has been proposed for the 2005 version of the DGR (5) is: "An infectious substance, which is transported in a form that when exposure to it occurs, is capable of causing permanent disability, life threatening or fatal disease to humans or animals".


274 **Table 2.** Indicative examples of animal pathogens forbidden as diagnostic specimens that must
 275 be shipped as infectious substances affecting animals (UN 2900)

African horse sickness virus	<i>Mycoplasma mycoides</i> – Contagious bovine pleuropneumonia
African swine fever virus	Peste des petits ruminants virus
Avian paramyxovirus Type 1 – Newcastle disease virus	Rinderpest virus
Bluetongue virus	Sheep-pox virus
Classical swine fever virus	Goatpox virus
Foot and mouth disease virus	Swine vesicular disease virus
Lumpy skin disease virus	Vesicular stomatitis virus

276 Any infectious agent that can cause disease in humans or animals that has been amplified in culture and new or
 277 emerging pathogens must also be assigned to UN 2814 or UN 2900. The following is the IATA definition of
 278 amplification in culture:

279 *Cultures (laboratory stocks) are the result of a process by which pathogens are amplified or propagated in order*
 280 *to generate high concentrations, thereby increasing the risk of infection when exposure to them occurs. This*
 281 *definition refers to cultures prepared for the intentional generation of pathogens and does not include cultures*
 282 *intended for diagnostic and clinical purposes.*

283 The following flow chart summarises the classification of diagnostic samples.

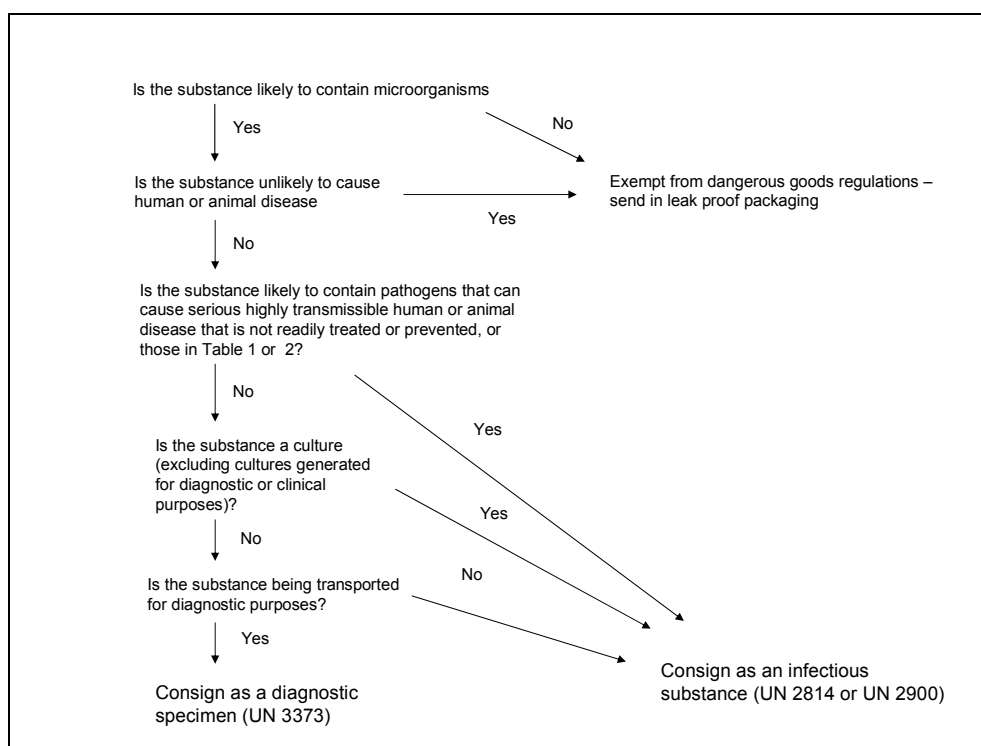

284
 285 The packaging of infectious substances and specimens from suspected serious animal diseases, UN 2814 or UN
 286 2900, are outlined in packing instruction 602; a Shippers Declaration of Dangerous Goods must be completed
 287 and submitted with these samples. There is also a requirement that the shipper receive training on the IATA-
 288 approved shipping procedures for UN 2814 and UN 2900 shipments. Due to the complexity of these guidelines
 289 the shipper is referred to the IATA regulations for further information on all UN 2814 or 2900 shipments.

290 The other group, UN 3373, covers 'Diagnostic Specimens'. This category has a lower risk and packages
 291 containing these specimens should be labelled as 'Diagnostic Specimens'; a Declaration of Dangerous Goods is
 292 not needed. IATA packing instruction 650 provides the guidelines for packaging infectious substances assigned to
 293 UN 3373 and the following is a summary of these packing instructions. However, the complete procedure, as
 294 outlined in the most recent IATA Dangerous Goods Regulations, must be followed (5, 6).

- 295 i) Infectious substances assigned to UN 3373 'Diagnostic Specimens' must be packed in good quality
296 packaging, which must be strong enough to withstand the shocks and loadings normally encountered during
297 transport. Packaging must be constructed and closed so as to prevent any loss of contents, which might be
298 caused under normal conditions of transport.
- 299 ii) The specimen should be put into the primary receptacle(s), which can be glass bottles, tubes or plastic
300 containers.
- 301 iii) Adequate adsorbent material must be packed around the primary receptacle(s) to absorb all the fluid in the
302 primary receptacle(s).
- 303 iv) If multiple primary receptacles are used they should be individually wrapped or separated so as to prevent
304 contact.
- 305 v) The primary receptacle(s), and adsorbent material, are put into the secondary receptacle.
- 306 vi) The primary receptacle and the secondary packaging used for liquids must be leak-proof. The primary
307 receptacle or secondary packaging must withstand, without leakage, an internal pressure differential of not
308 less than 95 kPa in the range from –40°C to 55°C.
- 309 vii) The primary receptacle(s) used for solids must not leak (be siftproof).
- 310 viii) The primary receptacle must not contain more than 500 ml of liquids or 500 g of solid specimens. The outer
311 packaging must not contain more than 4 litres for liquid specimens or 4 kg for solids.
- 312 ix) An itemised list of contents must be enclosed between the secondary packaging and the outer packaging.
- 313 x) If shipped at ambient temperatures or higher, the primary receptacle must have a positive means of ensuring
314 that it is leak proof, such as a leak proof seal, heat seal or skirted stopper. If screw caps are used they
315 should be taped shut.
- 316 xi) Prefrozen packs or dry ice can be packed around the secondary receptacle. If dry ice is used, there must be
317 an internal support to secure the secondary receptacle in the original position after the dry ice has been
318 dissipated. The outer packaging must permit the release of carbon dioxide. There are additional
319 requirements if liquid nitrogen is used and these are described in the DGR.
- 320 xii) The primary and secondary receptacles must be put into a shipping container with adequate cushioning
321 material.
- 322 xiii) The packaging must be able to withstand a 1.2 metre drop test. (There are additional strength requirements
323 for packaging used for UN 2900 and UN 2814 specimens.)
- 324 xiv) The package must be labelled Diagnostic Specimens. The 'Nature and Quantity of Goods' box of the airway
325 bill must state 'DIAGNOSTIC SPECIMENS PACKED IN COMPLIANCE WITH IATA PACKING
326 INSTRUCTION 650'.

327 **4. Shipping forms**

328 All shipping forms, including the import licence and submission form must be put in an envelope attached to the
329 outside of the shipping container. The forms and labels must be completed as outlined in the DGR and also put
330 on the outside of the container.

331 **E. PRESERVATION OF SAMPLES FOR PROLONGED STORAGE**

332 Establishing a collection of samples for future studies can be very useful. This can include cultures for comparison
333 with future isolates, tissue or serum samples that can be used for the validation of new tests and a collection of
334 fixed tissues, or paraffin blocks, for future histological examination. Possibly the most useful collection is the
335 storage of serum samples. These samples may be useful if a retrospective investigation is carried out to compare
336 the present disease status with that of earlier times.

337 **! Serum banks**

338 Serum samples can provide information about the animals from which the sera were taken. The samples can be
339 tested for a variety of constituents, such as immunoglobulins, trace elements, toxins, hormones and enzymes. If a
340 sufficient number of serum samples have been collected at random from a population, comparisons can be made
341 on the affect of sex, age, breed and geographical location. Results from this comparison can identify high risk
342 groups, vaccination priorities can be established, and patterns and rates of disease determined (7).

343 A serum bank is a catalogued collection of sera that are stored so as to preserve their immunological and other
 344 biochemical properties. Both the catalogue and the storage conditions are essential for a successful serum bank.
 345 Each individual sample should be fully documented and identified. The database should contain all relevant
 346 information about the origin of the sample and test results obtained. Additional data that may be of interest, such
 347 as weather conditions and the animal's productivity may also be included. Accurate records are essential and
 348 must be obtained when the blood samples are collected. The first essential is the complete identification of the
 349 animal. The amount of detail recorded should be appropriate to the abilities of the operator, accuracy being more
 350 important than quantity of information. Although pooling of sera reduces documentation and storage space, it
 351 should be avoided as it greatly reduces the usefulness of the material. Care should be taken to collect the blood
 352 as aseptically as possible and sterility should be maintained during separation of the serum and all other
 353 manipulations. The serum bank catalogue should be well organised and maintained on a computer database with
 354 appropriate backup. A suggested methodology has been described in detail (7).

355 Sera may be stored for periodic use or kept in long-term storage for historical purposes and these two functions
 356 should be separated. Storage conditions should minimise loss of immunological and other biochemical properties
 357 of the sera. There are three methods: deep freezing, dry storage on paper disks at ambient temperature and
 358 lyophilisation (freeze-drying). For long-term storage of sera by deep freezing, a core temperature below -60°C
 359 should be maintained. The lower the temperature the better, but lower temperatures are more expensive to
 360 maintain. Liquid phase N_2 is at -196°C , vapour phase N_2 is at -100°C and an ultra-low deep freezer will maintain
 361 -90°C . Some serum banks have been maintained at -20°C , but the serum may deteriorate and not be suitable for
 362 detection of some properties, especially if stored for long periods at this temperature. Deep-freezers should have
 363 a system to provide a warning if the temperature rises due to mechanical break down or power failure. A stand-by
 364 generator is essential together with alternative cold storage space in case the contents of a freezer must be
 365 transferred. Paper disk storage is a simple and inexpensive method, but it allows only a small quantity of serum to
 366 be stored and the eluted serum is only suitable for a limited number of tests. The disks should be kept in a cool,
 367 dry atmosphere. They can probably provide satisfactory results for up to about 5 years. Lyophilisation is generally
 368 regarded as the best method for long-term storage of sera. If freeze-drying conditions are optimised the loss of
 369 serum characteristics are minimised. Lyophilisation requires expensive equipment and is a time-consuming
 370 process. Lyophilised vials should be stored at 4°C .

371 REFERENCES

- 372 1. CAMERON A.R. & BALDOCK F.C. (1998). A new probability formula for surveys to substantiate freedom from
 373 disease. *Prev. Vet. Med.*, **34**, 1–17.
- 374 2. CANADIAN FOOD INSPECTION AGENCY, LABORATORY DIRECTORATE: ANIMAL HEALTH (2002). Manual of Common
 375 Procedures. Section: Specimen Collection and Submission; Specimen Packaging; Specimen Transportation.
 376 Canadian Food Inspection Agency, Ottawa, Canada, 61 pp.
- 377 3. CANNON R.M. & ROE R.T. (1982). Livestock Disease Surveys – A Field Manual for Veterinarians. Department
 378 of Primary Industry, Water and Environment, Australia, 15 pp.
- 379 4. COOK R., BARTON M., GLEESON L. & MAIN C. (1996). AUSVETPLAN Management Manual: Laboratory
 380 Preparedness. Animal Health Australia, Canberra, 56 pp. <http://www.aahc.com.au/ausvetplan/index.htm>.
- 381 5. INTERNATIONAL AIR TRANSPORT ASSOCIATION (2004). Dangerous Goods Regulations, 44th Edition.
 382 International Air Transport Association, 800 Place Victoria, P.O. Box 113, Montreal, Quebec H4Z 1M1,
 383 Canada, 801 pp.
- 384 6. INTERNATIONAL AIR TRANSPORT ASSOCIATION (2003). Infectious Agents and Diagnostic Specimens Shipping
 385 Guidelines, 4th Edition. IATA, 800 Place Victoria, P.O. Box 113, Montreal, Quebec H4Z 1M1, Canada, 208
 386 pp.
- 387 7. MOORHOUSE P.D. & HUGH-JONES M.E. (1981). Serum banks. *Vet. Bull.*, **51**, 277–290.
- 388 8. NATIONAL VETERINARY SERVICES LABORATORIES (2003). Procedures for Collection and Submission of
 389 Specimens. National Veterinary Services Laboratories, Ames, Iowa, USA. www.aphis.usda.gov/vs/nvsl.
- 390 9. OFFICE INTERNATIONAL DES EPIZOOTIES (2003). Terrestrial Animal Health Code. Office International des
 391 Epizooties, Paris, France. www.oie.int.
- 392 10. STRAFUSS A.C. (1988). Necropsy: Procedures and Basic Diagnostic Methods for Practicing Veterinarians.
 393 Charles C. Thomas, Springfield, IL, USA, 244 pp.

394 11. VETERINARY LABORATORIES AGENCY (1998). Submission of Samples to VI Centres. Veterinary Laboratories
395 Agency, New Haw, Addlestone, Surrey, United Kingdom, 36 pp.

396 12. WORLD HEALTH ORGANIZATION/FOOD AND AGRICULTURE ORGANIZATION OF THE UNITED NATIONS (WHO/FAO)
397 (1994). Basic Procedures for Veterinary Laboratories in Developing Countries, Pini A., Parodi P.,
398 Demeneghi D., Belemu U., Kabilika H. & Ghirotti M., eds. WHO/FAO Collaborating Centre, Viale Regina
399 Elena 299, 00161 Rome, Italy, 142 pp.

400 *

401 * *